

O₂ SL SENSOR + 4-20mA TRANSMITTER



Figure 1. Side view
O₂ SL sensor with
4-20mA transmitter
and installation kit.



Figure 2. Top view
O₂ SL Oxygen sensor with
4-20mA transmitter and
installation kit. Part no.
2112B4532



Figure 3. Components
O₂ transmitter with sinter
metal disc and blue
installation ring

SPECIFICATION

Operating Principle:	2-electrode cell
Measuring Range:	0-25% v/v
Output Signal:	4-20 mA
Response Time t90:	< 10 sec
Repeatability:	<± 1% of measuring signal
Long Term Output Drift:	<± 2% of signal per month
Temperature Range:	-20 °C to +50°C
Temperature Co-efficient:	<± 2% of signal per °C
Humidity Range:	15-90% relative humidity, non-condensing
Pressure Range:	1 atm ± 10%
Pressure Co-Efficient:	<± 0.003% of signal per mBar
Expected Operating Time:	18 months in air
Power Supply:	24 V d.c. ± 15%



**Figure 4. O₂ Gas
Measuring System**

The O₂ SL Oxygen sensor with
4-20mA transmitter and
installation kit is also available
as a complete housed unit in
aluminium housing.
Measuring range: 0-25% volume.
Part no. 2112B4533



O₂ SL SENSOR + 4-20mA TRANSMITTER

Potentiometer

for calibration adjustment

Please note: No zero adjustment required as automatically compensated

Test Gas

For calibration, flow required level of Oxygen O₂ through a test flow cap. Test Gas Cap and Calibration Gases also available from Euro-Gas. Please ask for details

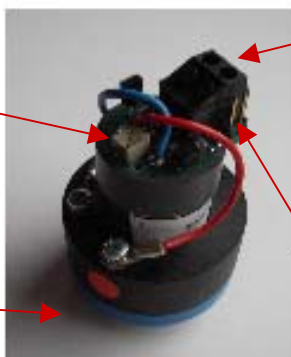


Figure 5. Instructions
O₂ SL Oxygen sensor
with 4-20mA transmitter
and installation kit.
Part no. 2112B4532

Two wire screw terminal

for 24V d.c. power supply (+/-10%); +4-20mA signal output.

Please note: No polarity (+/-) requirements

Test pins for one man calibration;
0.4 – 2.0 volts signal output



Figure 6. Test gas cap
Part no. 2112B1010

Two wire screw terminal: The transmitter has a two wire screw terminal to connect a 24V d.c. power supply. There is no polarity requirement across the two screw terminals (i.e. there is no +/- logic).

On the same two wires, you will receive the 4-20 mA signal output. The transmitter is precalibrated. When there is zero O₂ concentration, you will receive a 4mA signal. With a 25% volume concentration, you will receive a 20mA signal.

Potentiometer: This is used for adjusting the signal to the correct value if you apply a test gas concentration to the transmitter and it gives an incorrect signal.

Test pins: The two test pins allow for one man calibration. Please kindly note that the signal here is not 4-20 mA but **0.4 – 2.0 Volts**.

The data contained in this document is believed to be accurate and reliable. The data given is for guidance only. Euro-Gas Management Services Ltd accepts no liability for any consequential losses, injury or damage resulting from the use of this datasheet or the information contained in it. Customers should test the sensors under their own conditions to ensure that the sensors are suitable for their own requirements and in accordance with the plans and circumstances of the specific project and any standards/regulations pertaining to the country in which the sensors will be utilised. This datasheet is not intended to form the basis of a contract and in the interest of product improvement, Euro-Gas reserves the right to alter design features and specifications without notice. 08/10

